




GE Healthcare Project Management GE Healthcare has made reasonable efforts to ensure this BIM file conforms to requirements of the applicable pre-installation manual. This BIM file was produced to assist with site planning and is not intended for construction or final building modeling. GE Healthcare is not responsible for any damages resulting from use of such file for construction or final building modeling purposes. Compliance with all applicable local, state, and federal laws and regulations is the responsibility of the customer or its designated architects and engineers. Please keep in mind the information in this BIM file is dynamic and is subject to change without notice. It is the responsibility of the customer or its designated architect(s) and engineer(s) to ensure they have the latest equipment or product information.

SENOGRAPHE ESSENTIAL - RENDERING

| Project number | 9-32 | |
|----------------|-------------|-------------------|
| Date | 07.FEB.2017 | A-1 |
| Drawn by | GENPACT | |
| Checked by | | Scale 12" = 1'-0" |

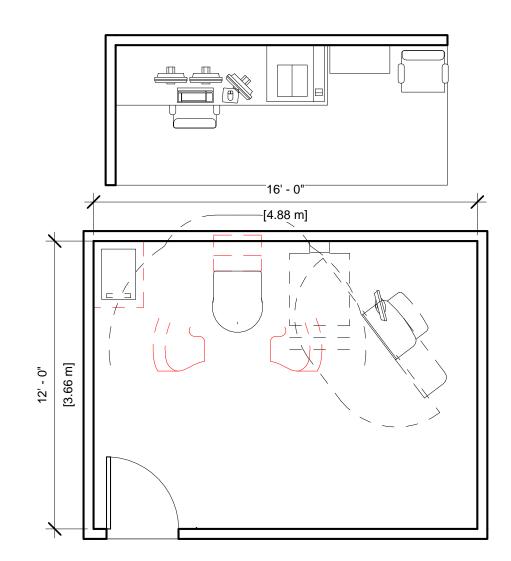

| Specialty Equipment Schedule | | | |
|--|--------------|------|--|
| Description | Weight (lbs) | BTU | |
| Control Room | | 1 | |
| REVIEW WORKSTATION | 134 | 2590 | |
| REVIEW WORKSTATION | 134 | 2590 | |
| REVIEW WORKSTATION | 134 | 2590 | |
| STORAGE CABINET | 48 | 0 | |
| UPS SYSTEM | 68 | 955 | |
| UPS SYSTEM | 68 | 955 | |
| COLOR PRINTER | 0 | 1054 | |
| CAD OPTION | 33 | 955 | |
| HYDRAULIC CHAIR | 0 | 0 | |
| Exam Room | | | |
| MAIN DISCONNECT CONTROL, WALL MOUNTED GEMS CAT. NO. E4502B, 65 lbs. SEE DETAIL R4502B. | 63 | 0 | |
| SENOGRAPHE ESSENTIAL GENERATOR | 352 | 3061 | |
| SENOGRAPHE ESSENTIAL GANTRY (BTU's INCLUDE CONTROL CONSOLE) | 789 | 341 | |
| SENOGRAPHE ESSENTIAL GANTRY (BTU's INCLUDE CONTROL CONSOLE) | 789 | 341 | |
| SENOGRAPHE ESSENTIAL CONTROL STATION | 462 | 0 | |
| SENOGRAPHE ESSENTIAL CONTROL STATION | 462 | 0 | |



GE Healthcare Project Management GE Healthcare has made reasonable efforts to ensure this BIM file conforms to requirements of the applicable pre-installation manual. This BIM file was produced to assist with site planning and is not intended for construction or final building modeling. GE Healthcare is not responsible for any damages resulting from use of such file for construction or final building modeling purposes. Compliance with all applicable local, state, and federal laws and regulations is the responsibility of the customer or its designated architects and engineers. Please keep in mind the information in this BIM file is dynamic and is subject to change without notice. It is the responsibility of the customer or its designated architect(s) and engineer(s) to ensure they have the latest equipment or product information.

SENOGRAPHE ESSENTIAL - PLAN & SCHEDULE

| Project number | 9-32 | |
|----------------|-------------|--------------------|
| Date | 07.FEB.2017 | A-2 |
| Drawn by | GENPACT | |
| Checked by | | Scale 1/4" = 1'-0" |

Hold the Left Click for Rotating around Use the Scroll for Zooming in and out



9-32 - Seno Essential



GE Healthcare

Click for Site Planning Support